

NBSIR 75-970 (R)
PB 253-252

EPA-600/2-76-126
May 1976

Environmental Protection Technology Series

*See verso of cover for other
non-NBS media*

DEVELOPMENT OF THIN CALIBRATION STANDARDS FOR X-RAY FLUORESCENCE ANALYSIS



Environmental Sciences Research Laboratory
Office of Research and Development
U.S. Environmental Protection Agency
Research Triangle Park, North Carolina 27711

RESEARCH REPORTING SERIES

Research reports of the Office of Research and Development, U.S. Environmental Protection Agency, have been grouped into five series. These five broad categories were established to facilitate further development and application of environmental technology. Elimination of traditional grouping was consciously planned to foster technology transfer and a maximum interface in related fields. The five series are:

1. Environmental Health Effects Research
2. Environmental Protection Technology
3. Ecological Research
4. Environmental Monitoring
5. Socioeconomic Environmental Studies

This report has been assigned to the ENVIRONMENTAL PROTECTION TECHNOLOGY series. This series describes research performed to develop and demonstrate instrumentation, equipment, and methodology to repair or prevent environmental degradation from point and non-point sources of pollution. This work provides the new or improved technology required for the control and treatment of pollution sources to meet environmental quality standards.

Pella, P. A., Kuehner, E. C., Cassatt, W. A.,
Development of a particulate reference sample
on membrane filters for the standardization of
x-ray fluorescence spectrometers, (Proc. 24th
Annual Conf. on Applications of X-Ray Analysis,
Denver, CO, Aug. 6-8, 1975), Chapter in
Advances in X-Ray Analysis, R. W. Gould,
C. S. Barrett, J. B. Newkirk and C. O. Ruud,
Eds., 19, 463-472 (Kendall/Hunt Publ. Co.,
Dubuque, Iowa, 1976).

Pella, P. A., Kuehner, E. C., Cassatt, W. A.,
Development of thin calibration standards for
x-ray fluorescence analysis, Environmental
Protection Technology Series, EPA-600/2-76-126,
11 pages (available as PB253252 from the
National Technical Information Service,
Springfield, Va., 22151, May 1976).

forma-

230

NBSIR 75-970(R)

310

16065

May 1976

DEVELOPMENT OF THIN CALIBRATION STANDARDS
FOR X-RAY FLUORESCENCE ANALYSIS

by

P. A. Pella, E. C. Kuehner, and W. A. Cassatt
National Bureau of Standards
Washington, DC 20234

Contract No. EPA-IAG-100(D)
DPA-IAG-D4-F849

Project Officer

T. G. Dzubay
Atmospheric Chemistry and Physics Division
Environmental Sciences Research Laboratory
Research Triangle Park, NC 27711

U.S. ENVIRONMENTAL PROTECTION AGENCY
OFFICE OF RESEARCH AND DEVELOPMENT
ENVIRONMENTAL SCIENCES RESEARCH LABORATORY
RESEARCH TRIANGLE PARK, NC 27711

DISCLAIMER

This report has been reviewed by the Environmental Science Research Laboratory, U.S. Environmental Protection Agency, and approved for publication. Approval does not signify that the contents necessarily reflect the views and policies of the U.S. Environmental Protection Agency, nor endorsement or recommendation for use.

I

INTRODUCTION

Within the past several years, an increasing number of x-ray analyses of environmental and biological samples have been reported in which the National Bureau of Standards Standard Reference Material (SRM) 1571 orchard leaves was used as a trace element calibration standard [1-3]. This botanical SRM is well suited to such applications because it contains a number of trace elements such as S, Cl, K, Ca, Cr, Mn, Fe, Co, Ni, Cu, Zn, As and Pb which are important in the analysis of environmental samples. In the analysis of ambient air particulates, the sample analyzed is often in the form of thin deposits on either membrane or Whatman type filters. Therefore, it is desirable to have a calibration sample in the same form. The preparation of orchard leaf deposits on membrane filters to be used for this purpose is described in this report.

The NBS SRM as certified requires that at least 250 mg samples be taken to insure that the trace element distribution is representative of the bulk material. To permit smaller samples to be used and to minimize the attenuation of x-rays in the individual particles, the material was reground. A number of different coatings were investigated to provide good sample protection, and at the same time obtain low attenuation of the x-rays from elements such as phosphorus and sulfur. Different coating materials that were investigated consisted of polyisobutylene, heat-sealed overlays of polypropylene and Parafilm, and vapor-deposited Parylene films.

EXPERIMENTAL

Sample deposits were prepared by filtration of a suspension of the reground material in cyclohexane. Attempts were made to prepare deposits from an aerosol suspension, but were not successful.

A. Grinding of the Orchard Leaves SRM 1571

A high velocity air impact grinder was used to reduce the particle sizes. The impactor produces two size fractions having relatively broad size distributions. The "fines" fraction was collected after each pass through the grinder and was reground four times. The particle size distribution of the collected material was characterized by automated image analysis. Data were taken by examining nine regions of four different sample preparations. These samples were prepared by dispersing a few milligrams of material in cyclohexane with ultrasonic stirring. About three drops of this suspension were placed on a microscope slide, covered with a cover glass and allowed to dry.

B. Preparation of Deposits on Membrane Filters

From 2 to 15 mg of dried reground orchard leaves were weighed and transferred to a 50 ml beaker containing about 40 ml of spectrograde cyclohexane. The beaker containing the orchard leaves was placed in an

ultrasonic bath for about one minute to disperse the particles. The suspension was transferred to a vacuum filtering unit and the sides of the beaker were washed down with cyclohexane. The material was filtered rapidly through a 37 mm preweighed membrane filter (0.8 μ m pore size). The glass filtering funnel was constructed so that deposits on the 37 mm membrane filters were 29 mm in diameter. The net weight of the air-dried deposit was used to calculate the areal density of the deposit in mg/cm². All weighings were performed in a room in which the relative humidity was maintained at 50 \pm 4 percent.

C. Preparation of Parylene-Coated Samples

The samples were coated at the Union Carbide Corporation with a thin film of Parylene N — a polymeric material developed by Union Carbide Corporation (U.S. Patent No. 3342754). The procedure consists of first vaporizing the di-para-xylylene dimer by heating it at 175°C at 760 mm Hg (1.01x10⁵ N/m²). This vaporized material passes through a deposition chamber maintained at room temperature, and 0.1 mm Hg (13.3 N/m²) which contains the samples to be coated. The samples are rotated in the chamber to insure a uniform coating of Parylene. The exit of the deposition chamber is connected to a cold trap (-70°C) and pumped with a mechanical pump to a pressure of 0.001 mm Hg (0.133 N/m²). The film thickness is monitored in the deposition chamber using a piezoelectric frequency sensor. More accurate thickness measurements were made at Union Carbide after removal of the samples using a UV spectrophotometer. The thickness is calculated from a calibration curve by comparing the absorbance of the film with that of a film of known thickness measured interferometrically.

D. Preparation of Thin-Film Overlays of Parafilm and Polypropylene

A sheet of Parafilm (American Can Co.) was stretched by hand as thinly as possible without causing the sheet to tear, and was placed directly on the sample which was held by suction to a filtering funnel. A polypropylene sheet (0.08 mm thick) was next placed on top of the Parafilm and was heat-sealed to the sample using a hot air gun.

E. Mounting the Parylene-Coated Filter Deposit

Filter holders for mounting the deposits were supplied by EPA, and are described in an EPA report [4]. These holders, designed to accommodate 37 mm diameter membrane filters, were modified by increasing the platform diameter by 2 mm. This permitted the filter deposit to be centered in the holder more easily and also allowed for some expansion of the membrane filter before cementing in the holder. The filter deposit was held on a filtering funnel by applying suction. A thinned mixture of cement prepared by mixing equal parts of Barge all-purpose cement, ethyl acetate and cyclohexane was brushed on the platform of the holder. The filter was cemented to the holder platform by pressing the holder flat against the outer edge of the filter deposit and then allowed to dry.

RESULTS AND DISCUSSION

Neutron activation analysis (NAA) of the reground orchard leaves showed that the concentrations of iron, nickel, cobalt and chromium were much higher than in the certified SRM 1571. Therefore, it was important to determine if these introduced elements were homogeneously distributed throughout the material. For this reason, sixteen samples of reground material (200 mg each) were taken and six elements, including iron and chromium, were analyzed by NAA. An analysis of variance of these concentrations in the material indicated that there were no gross inhomogeneities (not greater than five percent). These results indicated that the reground SRM 1571 was satisfactory for use provided that recertification of the introduced elements could be accomplished. An analysis of a number of these elements using NAA, atomic absorption spectrophotometry (AAS), and photon activation analysis (PAA) are included at the end of this report. Further work on the analysis of this material is still in progress.

The particle size distribution of the reground material is shown in figure 1. The area of about 80 percent of the 3000 particles examined was between zero and $7.5 \mu\text{m}^2$ ($3.1 \mu\text{m}$ equivalent diameter). Less than 0.5 percent of the particles were within 82.5 and $105 \mu\text{m}^2$, with no particles observed above $105 \mu\text{m}^2$.

To determine if the cyclohexane treatment altered the trace element composition of the orchard leaves, NAA was performed on cyclohexane extracts and on the material after treating with cyclohexane. A number of elements, including Br, Mn, Fe, K and Na, were analyzed. The results showed that only sodium was affected by this treatment, and about 50 percent was extracted.

A simple technique was developed for measuring the uniformity of the deposits. This consisted of directing a laser beam about 2 mm in diameter normal to the sample, and measuring the intensity of the light transmitted [5]. Using a Beer's law calibration of absorbance vs areal density, the uniformity of the deposit was measured. Of the several samples examined having areal densities of 1.0 to 2.0 mg/cm^2 , variations in uniformity did not exceed 0.02 mg/cm^2 .

A number of coating materials were investigated and compared with regard to their ability to adhere to the sample and to provide protection from abrasion and humidity. These consisted of vapor-deposited Parylene films and heat-sealed overlays of polypropylene using Parafilm as a binder. Also, orchard leaf deposits were prepared from suspensions in cyclohexane containing from 0.1 to 10 percent by weight of polyisobutylene. Another important factor considered was the x-ray attenuation of these coatings, especially from elements of low atomic number such as phosphorus and sulfur. The attenuation of P, S, K, and $\text{CaK}\alpha$ lines was measured by comparing the background corrected peak intensities of coated and uncoated samples having the same areal densities using a wavelength-dispersive x-ray spectrometer.

The values obtained for various thicknesses of Parylene and of thin polypropylene and Parafilm coatings are summarized in tables 1 and 2, respectively. For Parylene coatings 75 to 193 nm thick, little change in attenuation was noted. Also, the x-ray background intensities from these samples were essentially the same as the uncoated samples except that the background of the 2500 nm thick sample was increased significantly. The attenuation values of the polypropylene-Parafilm coatings could not be reduced any further because thinner films were not available. In order to produce adherent deposits using polyisobutylene, as much as one percent or greater by weight of the polymer in cyclohexane was used. However, the amount of polyisobutylene retained on the samples varied considerably making it difficult to obtain reproducible attenuation data. For this reason, this coating material was considered unsatisfactory.

Table 1. Average Attenuation Values of Parylene Coatings^a

sample areal density = 2.0 mg/cm ²				
<u>No. of Samples</u>	<u>Parylene Thickness, nm</u>	<u>Percent Attenuation</u>		<u>S^b</u>
		<u>Element</u>	<u>Average</u>	
5	75	P	3	1.7
3	75	S	2	1.3
2	75	K	1.4	--
5	117.5	P	3.1	0.50
5	117.5	K	1.7	0.44
5	158.0	P	5.4	0.90
2	158.0	S	5.2	--
4	158.0	K	2.9	0.35
7	166.5	P	5.0	0.81
5	166.5	S	4.3	0.92
7	166.5	K	2.6	0.69
5	193.0	P	7.3	0.88
3	193.0	K	3.7	0.20
3	2500	P	33	1.5
3	2500	S	28.9	0.71
2	2500	K	11.4	--

^aCalculated from the expression $(I_u - I_c)/I_u \times 100$; where I_u = peak intensity of uncoated sample, and I_c = peak intensity of coated sample.

^bS = standard deviation of a single measurement.

Table 2. Attenuation Values of Polypropylene
and Parafilm Coatings

<u>Sample #</u>	<u>Total Coating Thickness, mg/cm²</u>	<u>Percent Attenuation</u>				
		<u>P</u>	<u>S</u>	<u>Cl</u>	<u>K</u>	<u>Ca</u>
1	1.2	28.1	23.2	14.1	10.9	8.5
2	1.1	24.4	23.6	16.2	11.4	7.9
3	1.2	26.3	24.4	13.6	10.1	8.3
Average		26.3	23.7	14.6	10.8	8.2

The ruggedness of samples coated with Parylene films (75 to 200 nm thick) were tested by an air jet which impinged on the sample surface. Effects of humidity were observed when the samples were placed in a chamber maintained at 100 percent relative humidity.

The trace element composition of the starting material (di-para-xylylene dimer) was analyzed at Union Carbide Corporation. Of the 27 elements analyzed, sodium, magnesium, iron and aluminum were present in concentrations from 2 to 9 ppm. Silicon was 31 ppm, and the remaining elements were either below 1 ppm or were not detected. These results indicate that the Parylene material should be of sufficient purity for application in this work. Since the Parylene films appeared to furnish good sample protection, including high resistance to humidity, high purity, good adherence, and acceptable x-ray attenuation for the low atomic number elements, 60 samples were prepared and delivered to EPA containing from 0.1 to 5.0 mg/cm² of orchard leaves coated with 117.5 nm of Parylene.

A photograph of a typical reference sample mounted in a holder is shown in figure 2.

Table 3. Preliminary Results of the Analysis
of Reground SRM 1571 Orchard Leaves

<u>Element</u>	<u>No. of Meas.</u>	<u>Average, $\mu\text{g/g}$</u>	<u>Rel. Std. Dev. %</u>	<u>Certified Values of SRM 1571, $\mu\text{g/g}$</u>
Fe ^a	3	791	0.2	300±20
Ni ^a	3	22.5	0.5	1.3±0.2
Ni ^b	1	21.5	---	
Cr ^c	15	41.97	3.70	(2.3)
Mn ^c	16	102.1	1.84	91±4
K ^c	16	1.49 (wt. %)	1.53	1.47±0.03 (wt. %)
Br ^c	15	10.48	2.58	(10)
Zn ^c	15	24.99	3.22	25±3

^a = AAS

^b = PAA

^c = NAA

Values in parenthesis are not certified.

II

CONCLUSIONS

Reference samples consisting of uniform layers of reground orchard leaves of known composition, i.e., NBS SRM 1571, on membrane filters were prepared for the standardization of x-ray fluorescence spectrometers. These samples have areal densities of 0.1 to 5.0 mg/cm², and are coated with a thin polymer film for protection against abrasion and moisture.

REFERENCES

1. J. A. Cooper, Nucl. Instr. and Meth. 106, 525 (1973).
2. R. D. Giaque, F. S. Goulding, J. M. Jaklevic and R. H. Pehl, Anal. Chem. 45, 671 (1973).
3. F. W. Reuter, III, Anal. Chem. 47, 1763 (1975).
4. F. S. Goulding and J. M. Jaklevic, EPA Report No. EPA-R2-73-182, April 1973.
5. E. C. Kuehner and W. A. Cassatt, A Laser Microphotometer for Determining Uniformity of Particulate Deposits on Membrane Filters, in press.

Identification of any commercial product does not imply recommendation or endorsement by the National Bureau of Standards, nor does it imply that the material or equipment identified is necessarily the best available for the purpose.

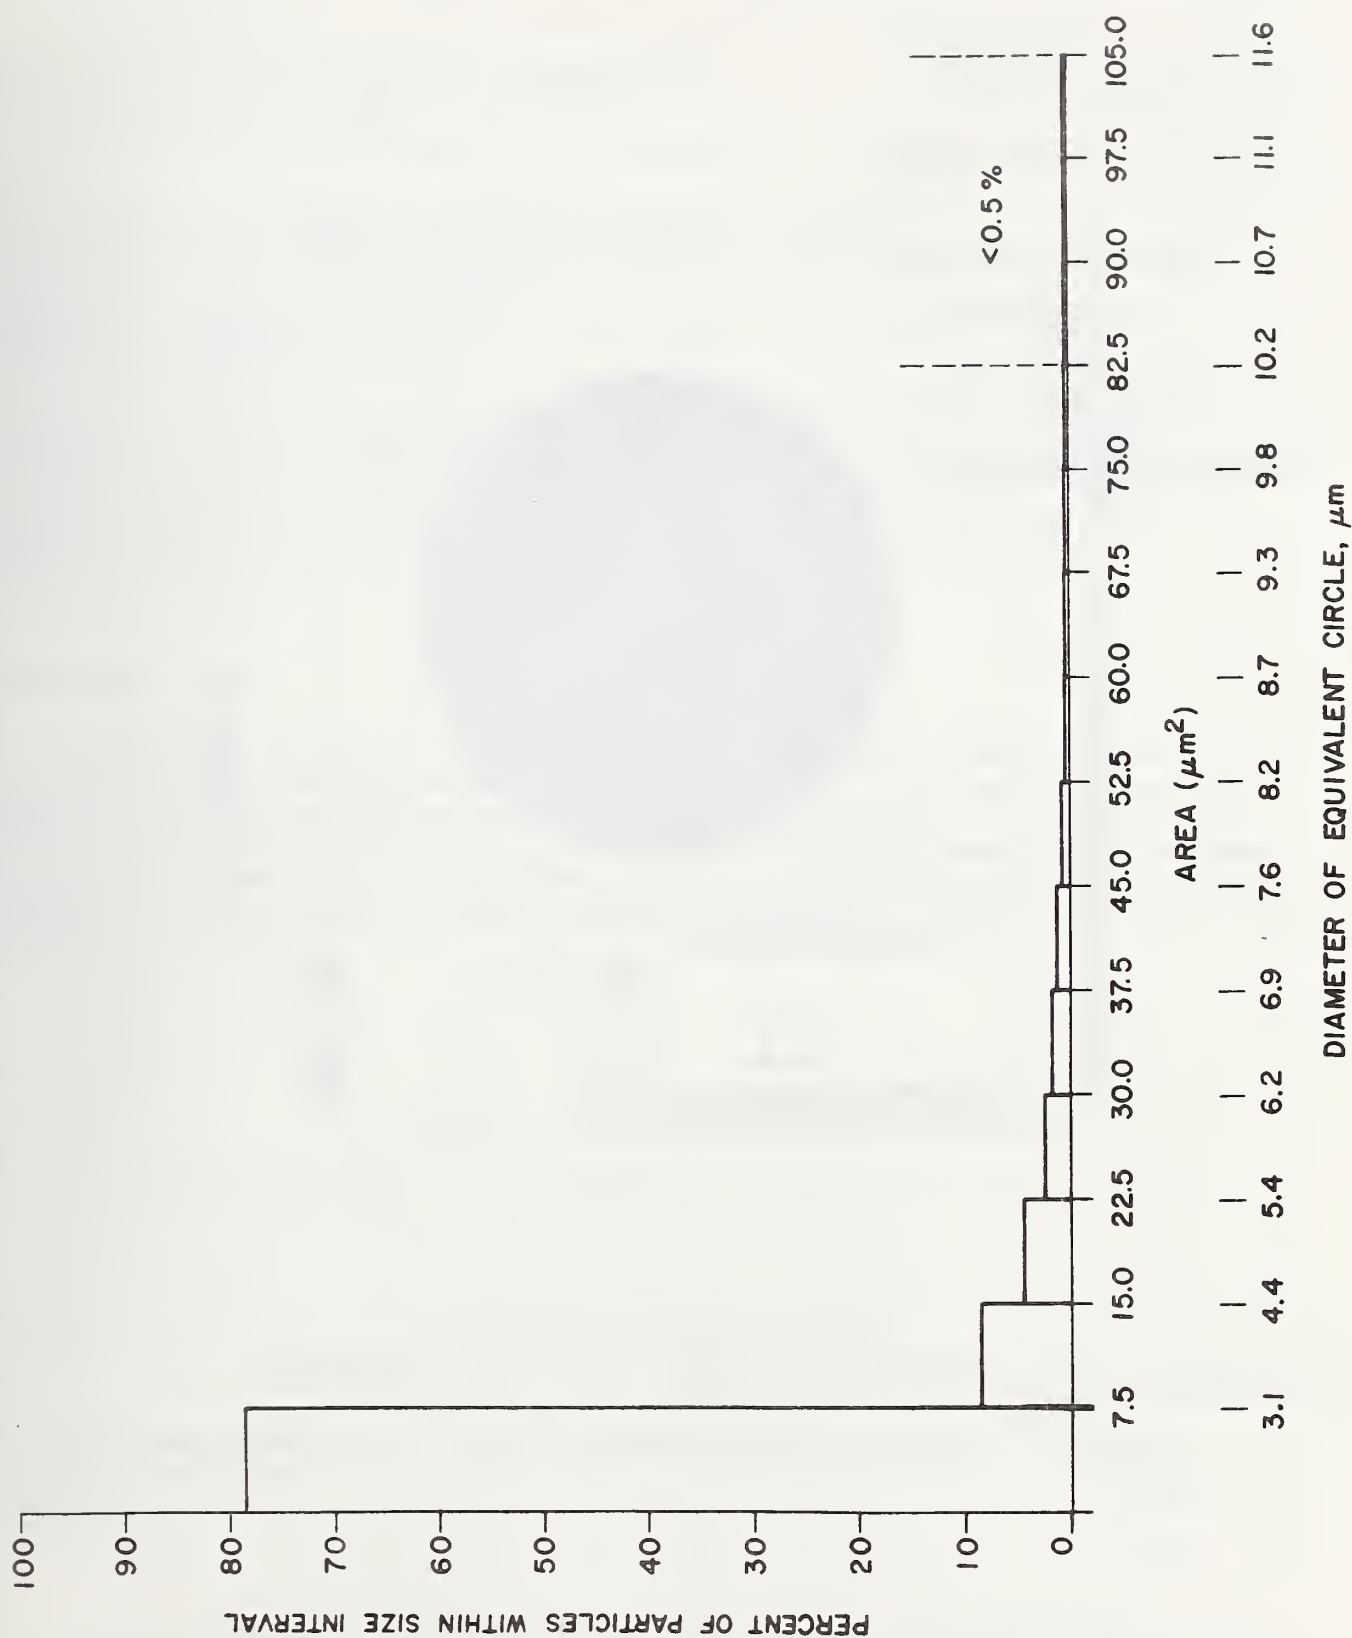


Figure 1. Particle size distribution of orchard leaves.



Figure 2. Reference sample mounted in holder (actual size 5x5 cm).

TECHNICAL REPORT DATA
(Please read Instructions on the reverse before completing)

1. REPORT NO. EPA-600/2-76-126		2.		3. RECIPIENT'S ACCESSION NO.	
4. TITLE AND SUBTITLE DEVELOPMENT OF THIN CALIBRATION STANDARDS FOR X-RAY FLUORESCENCE ANALYSIS				5. REPORT DATE May 1976	
				6. PERFORMING ORGANIZATION CODE	
7. AUTHOR(S) P. A. Pella, E. C. Kuehner, and W. A. Cassatt				8. PERFORMING ORGANIZATION REPORT NO.	
9. PERFORMING ORGANIZATION NAME AND ADDRESS Analytical Chemistry Division National Bureau of Standards Washington, DC 20234				10. PROGRAM ELEMENT NO. 1A1010	
				11. CONTRACT/GRANT NO. EPA-IAG-100 (D) DPA-IAG-D4-F849	
12. SPONSORING AGENCY NAME AND ADDRESS Environmental Science Research Laboratory Office of Research and Development U. S. Environmental Protection Agency Research Triangle Park, NC 27711				13. TYPE OF REPORT AND PERIOD COVERED Final 6/1/7/74 - 6/1/75	
				14. SPONSORING AGENCY CODE EPA-ORD	
15. SUPPLEMENTARY NOTES					
16. ABSTRACT <p>Particulate reference samples have been prepared for the standardization of X-ray fluorescence spectrometers used in the analysis of air particulate matter. Uniform layers of reground orchard leaves of known composition, i.e., National Bureau of Standards Standard Reference Material 1571, were deposited on membrane filters and coated with a thin polymer film for protection against abrasion and moisture. These samples have been prepared with mass per unit area of 0.1 to 5.0 mg/cm .</p>					
17. KEY WORDS AND DOCUMENT ANALYSIS					
a. DESCRIPTORS		b. IDENTIFIERS/OPEN ENDED TERMS		c. COSATI Field/Group	
* X-ray fluorescence * Chemical analysis * Standards Calibrating				20F 07D 14B	
18. DISTRIBUTION STATEMENT RELEASE TO PUBLIC		19. SECURITY CLASS (This Report) UNCLASSIFIED		21. NO. OF PAGES 13	
		20. SECURITY CLASS (This page) UNCLASSIFIED		22. PRICE	

INSTRUCTIONS

1. **REPORT NUMBER**
Insert the EPA report number as it appears on the cover of the publication.
2. **LEAVE BLANK**
3. **RECIPIENTS ACCESSION NUMBER**
Reserved for use by each report recipient.
4. **TITLE AND SUBTITLE**
Title should indicate clearly and briefly the subject coverage of the report, and be displayed prominently. Set subtitle, if used, in smaller type or otherwise subordinate it to main title. When a report is prepared in more than one volume, repeat the primary title, add volume number and include subtitle for the specific title.
5. **REPORT DATE**
Each report shall carry a date indicating at least month and year. Indicate the basis on which it was selected (*e.g., date of issue, date of approval, date of preparation, etc.*).
6. **PERFORMING ORGANIZATION CODE**
Leave blank.
7. **AUTHOR(S)**
Give name(s) in conventional order (*John R. Doe, J. Robert Doe, etc.*). List author's affiliation if it differs from the performing organization.
8. **PERFORMING ORGANIZATION REPORT NUMBER**
Insert if performing organization wishes to assign this number.
9. **PERFORMING ORGANIZATION NAME AND ADDRESS**
Give name, street, city, state, and ZIP code. List no more than two levels of an organizational hierarchy.
10. **PROGRAM ELEMENT NUMBER**
Use the program element number under which the report was prepared. Subordinate numbers may be included in parentheses.
11. **CONTRACT/GRANT NUMBER**
Insert contract or grant number under which report was prepared.
12. **SPONSORING AGENCY NAME AND ADDRESS**
Include ZIP code.
13. **TYPE OF REPORT AND PERIOD COVERED**
Indicate interim final, etc., and if applicable, dates covered.
14. **SPONSORING AGENCY CODE**
Leave blank.
15. **SUPPLEMENTARY NOTES**
Enter information not included elsewhere but useful, such as: Prepared in cooperation with, Translation of, Presented at conference of, To be published in, Supersedes, Supplements, etc.
16. **ABSTRACT**
Include a brief (*200 words or less*) factual summary of the most significant information contained in the report. If the report contains a significant bibliography or literature survey, mention it here.
17. **KEY WORDS AND DOCUMENT ANALYSIS**
 - (a) **DESCRIPTORS** - Select from the Thesaurus of Engineering and Scientific Terms the proper authorized terms that identify the major concept of the research and are sufficiently specific and precise to be used as index entries for cataloging.
 - (b) **IDENTIFIERS AND OPEN-ENDED TERMS** - Use identifiers for project names, code names, equipment designators, etc. Use open-ended terms written in descriptor form for those subjects for which no descriptor exists.
 - (c) **COSATI FIELD GROUP** - Field and group assignments are to be taken from the 1965 COSATI Subject Category List. Since the majority of documents are multidisciplinary in nature, the Primary Field/Group assignment(s) will be specific discipline, area of human endeavor, or type of physical object. The application(s) will be cross-referenced with secondary Field/Group assignments that will follow the primary posting(s).
18. **DISTRIBUTION STATEMENT**
Denote releasability to the public or limitation for reasons other than security for example "Release Unlimited." Cite any availability to the public, with address and price.
19. & 20. **SECURITY CLASSIFICATION**
DO NOT submit classified reports to the National Technical Information service.
21. **NUMBER OF PAGES**
Insert the total number of pages, including this one and unnumbered pages, but exclude distribution list, if any.
22. **PRICE**
Insert the price set by the National Technical Information Service or the Government Printing Office, if known.